



Radiolucent Liver / Oncology System SUGGESTED SET UPS

Liver / Oncology / HPB

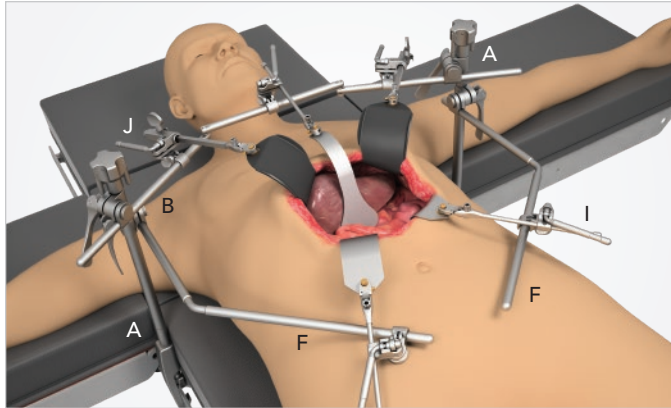

Lower Abdominal Oncology

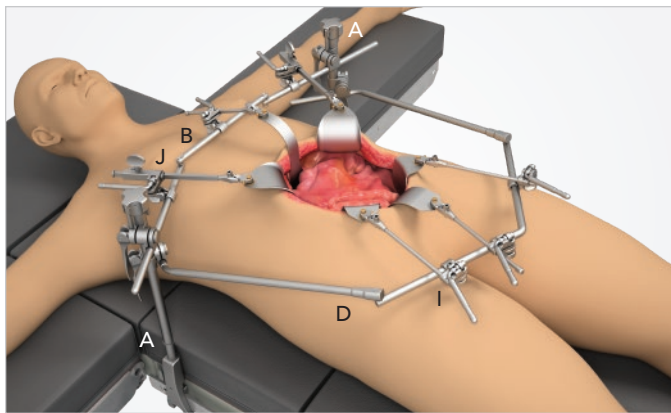

Additional suggested set ups shown on page 28.

(RADIO. LIVER / ONCOLOGY SYSTEM #SL82008 CONTINUED)

REF	PART #	ITEM DESCRIPTION	QTY
I	SL42126WGP	Cam II Clip-on Quick Angle 8"	6
J	SL45006CGP	Micro-Adjustable II Clip-on Quick Angle 10"	2
K	SL45006CGRP	Micro-Adjustable II Clip-on Quick Angle 15"	2
L	60020	T-Handle	2
	50000G	Instrument Case (23" x 11" x 3 1/2")	1
Tray 3			
M	SL46115ET	Malleable 13mm x 64mm (1/2" x 2 1/2")	2
N	SL46116ET	Malleable 13mm x 152mm (1/2" x 6")	2
	SL46117ET	Malleable 13mm x 203mm (1/2" x 8")	2
O	SL46118ET	Malleable 25mm x 203mm (1" x 8")	1
P	SL46118PET	Malleable 25mm x 104mm (1" x 4")	1
	SL46122ET	Malleable 51mm x 203mm (2" x 8")	1
P	SL46124ET	Malleable 64mm x 254mm (2 1/2" x 10")	2
	SO46124AET	Malleable 76mm x 254mm (3" x 10")	1
Q	SO46124BET	Malleable 102mm x 254mm (4" x 10")	1
R	SO46129ET	Kelly 64mm x 76mm (2 1/2" x 3")	1
	SO46130ET	Kelly 76mm x 89mm (3" x 3 1/2")	2
	SO46140CEB	Balfour [small lips] 65mm x 72mm (2 1/2" x 2 3/4")	1
S	SO46141EB	Balfour [lips] 83mm x 70mm (3 1/4" x 2 3/4")	2
T	SO46141CEB	Balfour [small lips] 83mm x 70mm (3 1/4" x 2 3/4")	2
U	SO46141DEB	Balfour [lips] 83mm x 127mm (3 1/4" x 5")	2
V	SL46142EB	Balfour [lips] 32mm x 32mm (1 1/4" x 1 1/4")	4
W	SL46153ET	Richardson 51mm x 178mm (2" x 7")	1
X	SL46160ET	Harrington 64mm x 152mm (2 1/2" x 6")	1
Y	SO46188ET	St. Marks [with lip] 64mm x 178mm (2 1/2" x 7")	1
Z	SL46191ET	Malleable Finger 152mm (6")	2
	SO46241AEB	Wide Balfour 83mm x 57mm (3 1/4" x 2 1/4")	1
1	SO46241BEB	Wide Balfour 100mm x 61mm (4" x 2 3/8")	1
	SO46241CEB	Wide Balfour 114mm x 63mm (4 1/2" x 2 1/2")	1
2	SO46170CEB	Non-Slip Balfour L 77mm x 94mm (3" x 3 3/4")	1
3	SO46171CEB	Non-Slip Balfour R 77mm x 94mm (3" x 3 3/4")	1
	50000G	Instrument Case (22" x 11" x 3 1/2")	1

RADIO. LIVER / ONCOLOGY SYSTEM #SL82008

REF	PART #	ITEM DESCRIPTION	QTY
Tray 1			
A	43903AC	Elite III Rail Clamp with 2 Cam Joints 18"	2
B	41900PH	34" Bilateral Crossbar Hinged 11 1/2" x 8 1/2" x 11 1/2"	1
C	41900F	Bilateral Crossbar 7 1/4" x 13 1/2" x 7 1/4"	1
D	44112SP	20" Lower Abdominal Bar (14" x 6")	1
	50000BL	Instrument Case	1
Tray 2			
E	44118N	18" Angled Arm (8" x 10") @ 45°	1
F	44124W	24" Angled Arm (11" x 13") @ 45°	2
G	44124N	24" Angled Arm (8" x 16") @ 45°	1
H	43112C	Cam III Joint Serrated 1/2" x 1/2"	2

Radiolucent Liver / Oncology System COMPONENTS

RETRACTOR SYSTEMS



Radiolucent blades eliminate the need to remove retraction during imaging.

“I am quicker, more dynamic and precise in my biliary procedures. In addition, I am essentially non-reliant on my assistant for exposure or retraction.”

- David Sindram, MD, PhD